



**Comments:** Perfect correlation and accuracy with similar average concentration and daily patterns. DQO is met above 28ppb.


**Version:** KUNAKAIR V2.5





# NITROGEN DIOXIDE (NO<sub>2</sub>), BARCELONA (Spain), FEB'19 – MAR'19

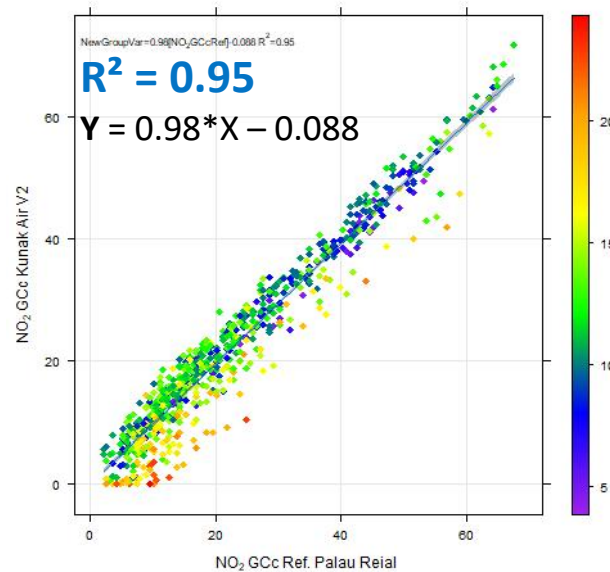


Time variation of Kunak Air V2 and Ref. Palau Reial : NO<sub>2</sub> GCc

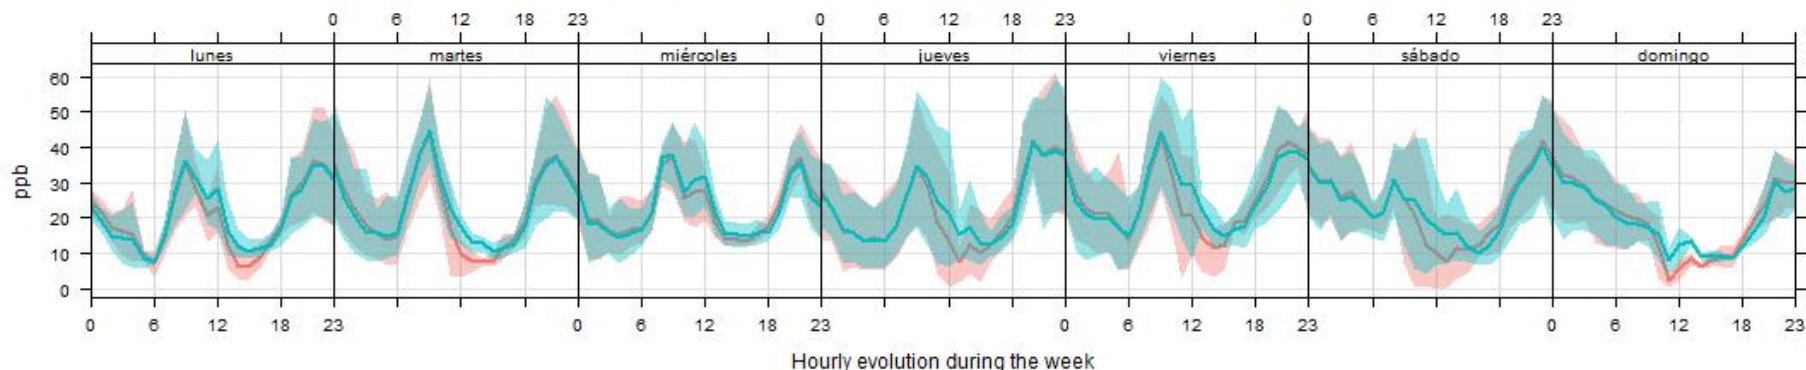

■ NO<sub>2</sub> GCc Kunak Air V2    
 ■ NO<sub>2</sub> GCc Ref. Palau Reial



Mean and 95% confidence interval in mean

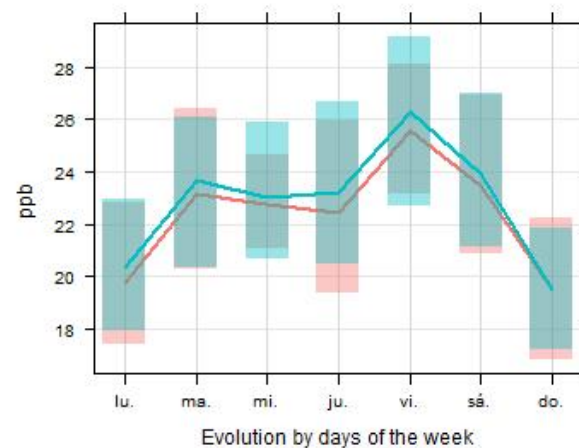

R <sup>2</sup>	ACCY (PPB)	90% CONF. (PPB)	DQO (PPB)	AVG. GC. REF (PPB)	AVG. GC. DUT (PPB)	AV REF/DUT
0.95	<b>2.66</b>	5.65	28	22.91	22.17	97.4% / 99.9%