
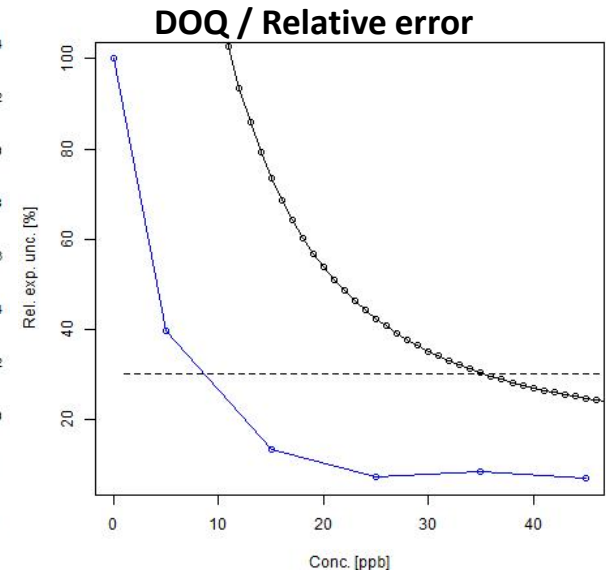


Comments: Please, note statistics are only shown after the Span calibration carried out on 20th February. After this calibration, excellent correlation and accuracy is met. DQO is met above 26ppb.


Same daily patterns as well as average concentration is detected for KUNAKAIR and Reference station.

Version: KUNAKAIR V2.5



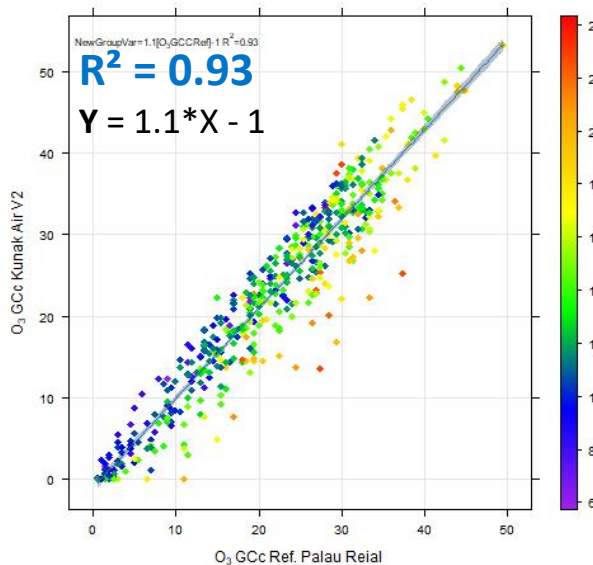


OZONE (O₃), BARCELONA (Spain), FEB'19 – MAR'19

Time variation of Kunak Air V2 and Ref. Palau Reial : O₃ GCc

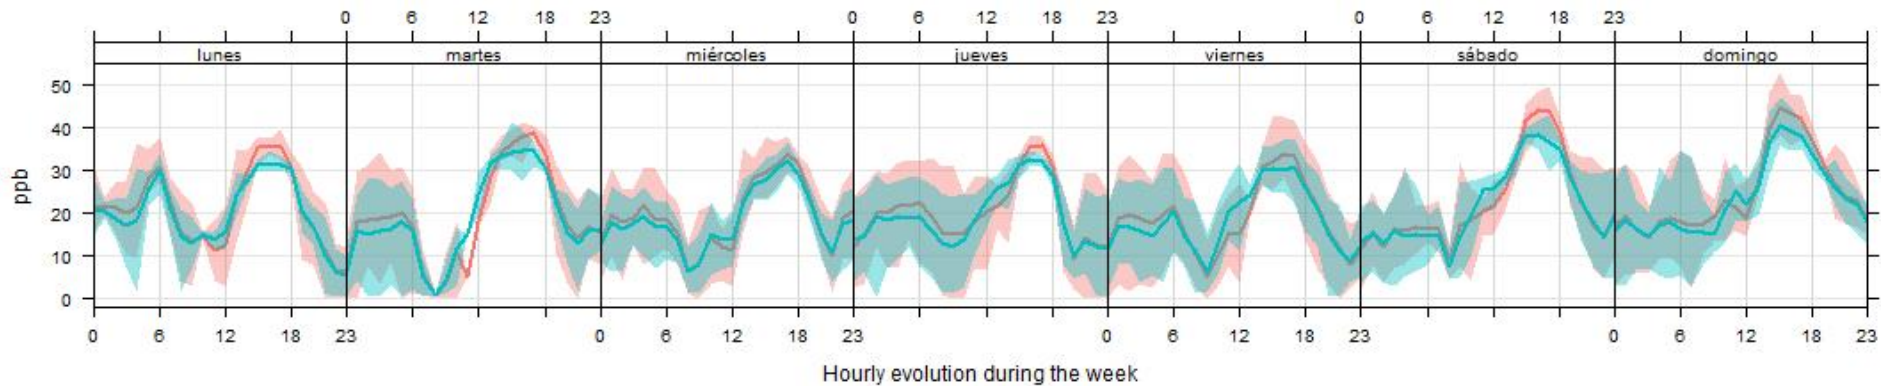

■ O₃ GCc Kunak Air V2 ■ O₃ GCc Ref. Palau Reial

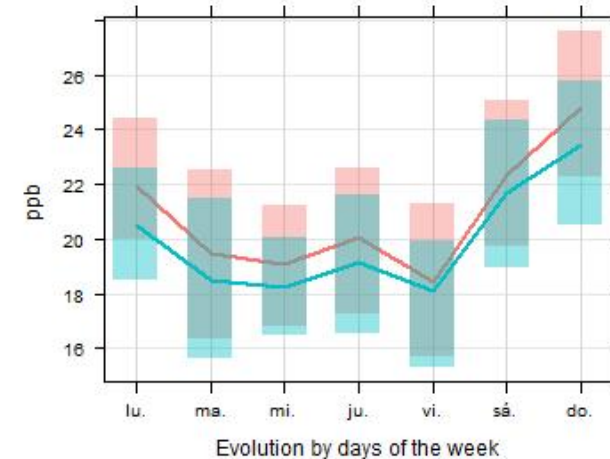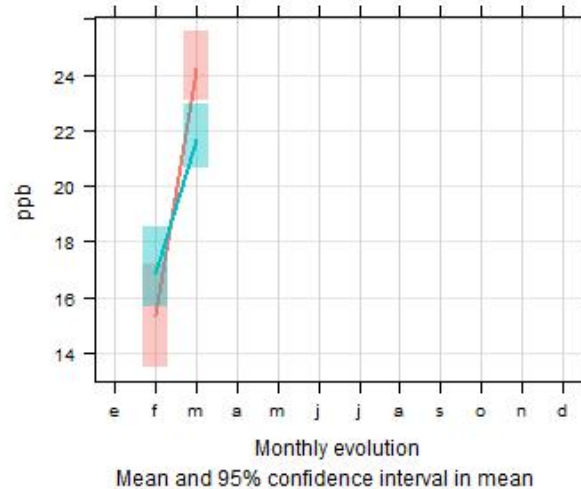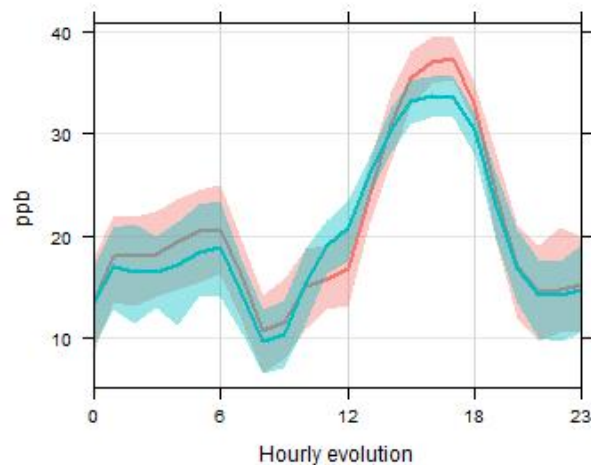

R ²	ACCY (PPB)	90% CONF. (PPB)	DQO (PPB)	AVG. GC. REF (PPB)	AVG. GC. DUT (PPB)	AV REF/DUT
0.93	2.94	6.05	26	19.8	20.71	97.4% / 99.9%