



NITROGEN DIOXIDE (NO₂), SABADELL (Spain), MAY'18-JUN'18

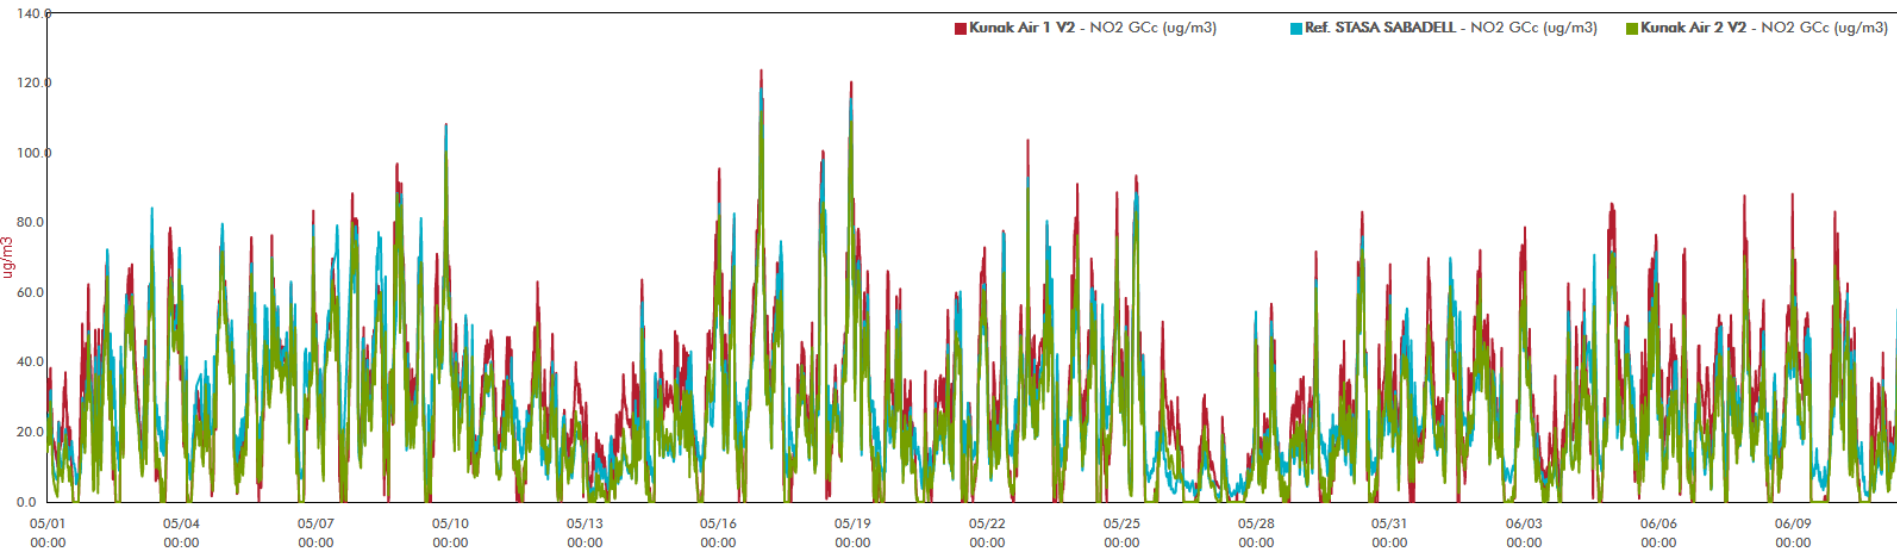


Comments: Excellent to good correlation between KUANKAIR and reference. Extremely linear at high concentration values for both devices. Time variation follows perfectly the reference station with pretty similar average results.

Version: KUNAKAIR V2.





Kunak Air 1 V2

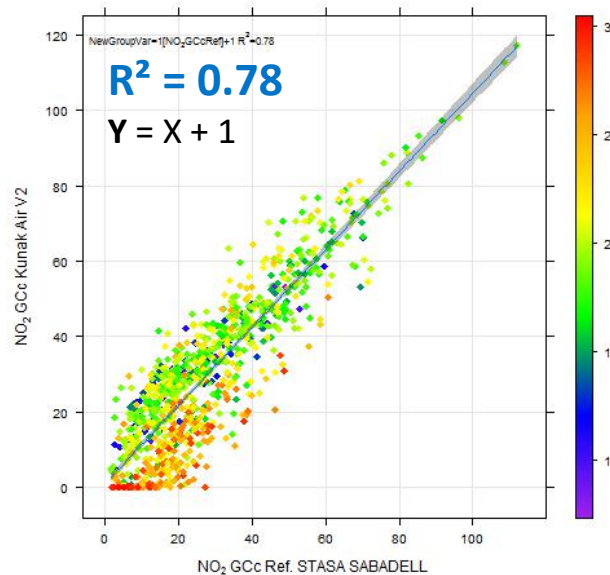

Kunak Air 2 V2

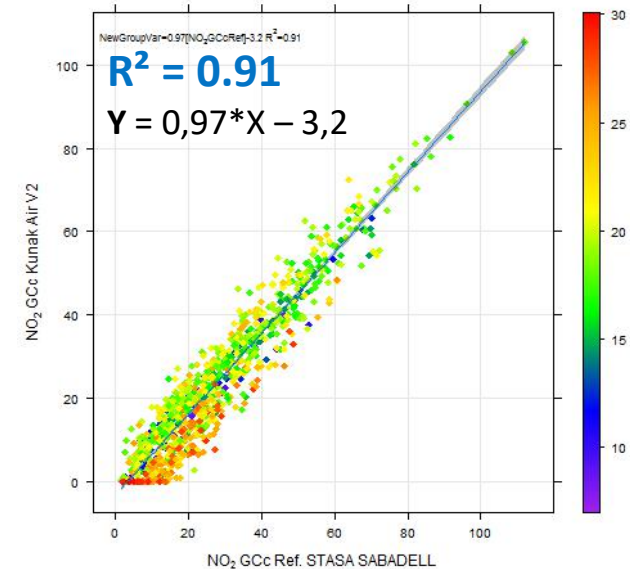

Time variation of two Kunak Air V2 and Ref. Torneo : NO₂ GCc

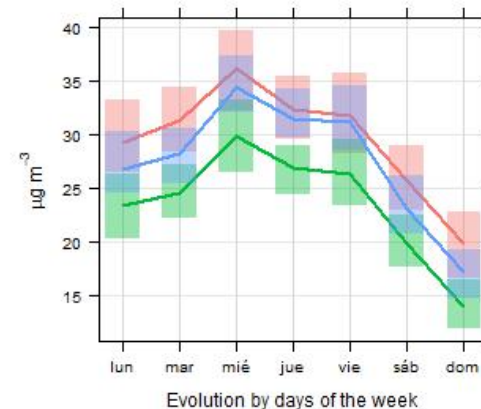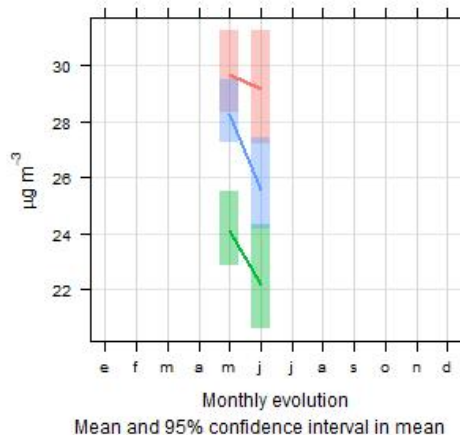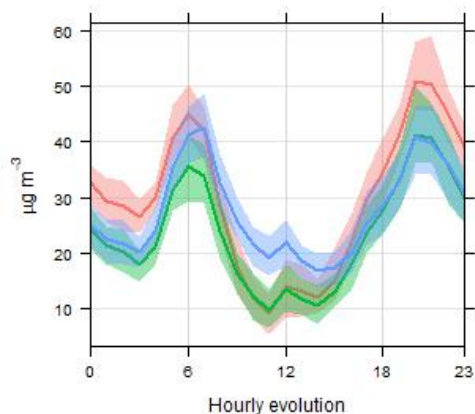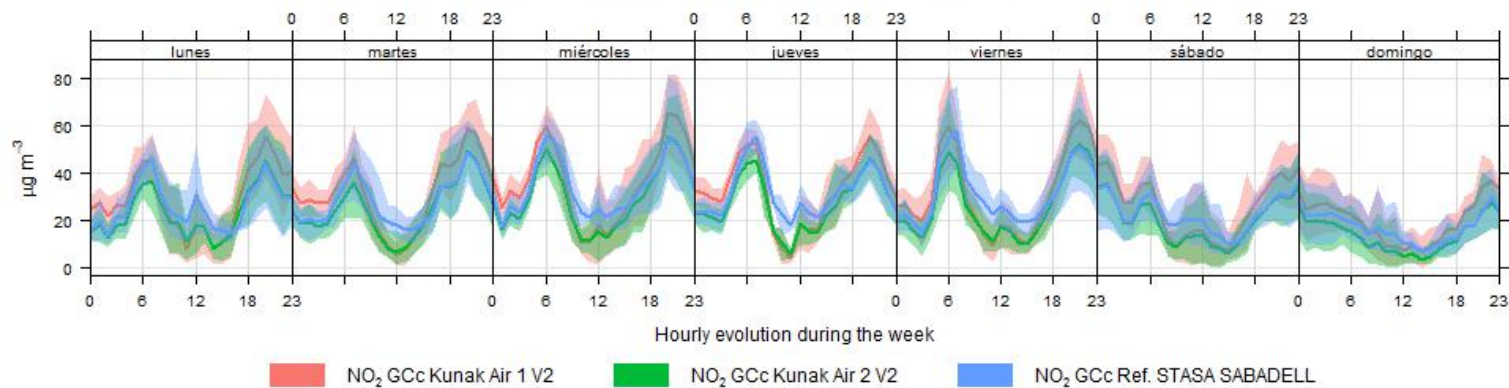

Device	R ²	ACCY (µg/m ³)	90% CONF. (µg/m ³)	AVG. GC. REF (µg/m ³)	AVG. GC. DUT (µg/m ³)	AV REF/DUT
KA 1	0.78	8.25	15.31	27.57	29.56	98.5/100
KA 2	0.91	5.23	11.45	27.57	23.63	98.5/100