



OZONE (O₃), SABADELL (Spain), MAY'18-JUN'18

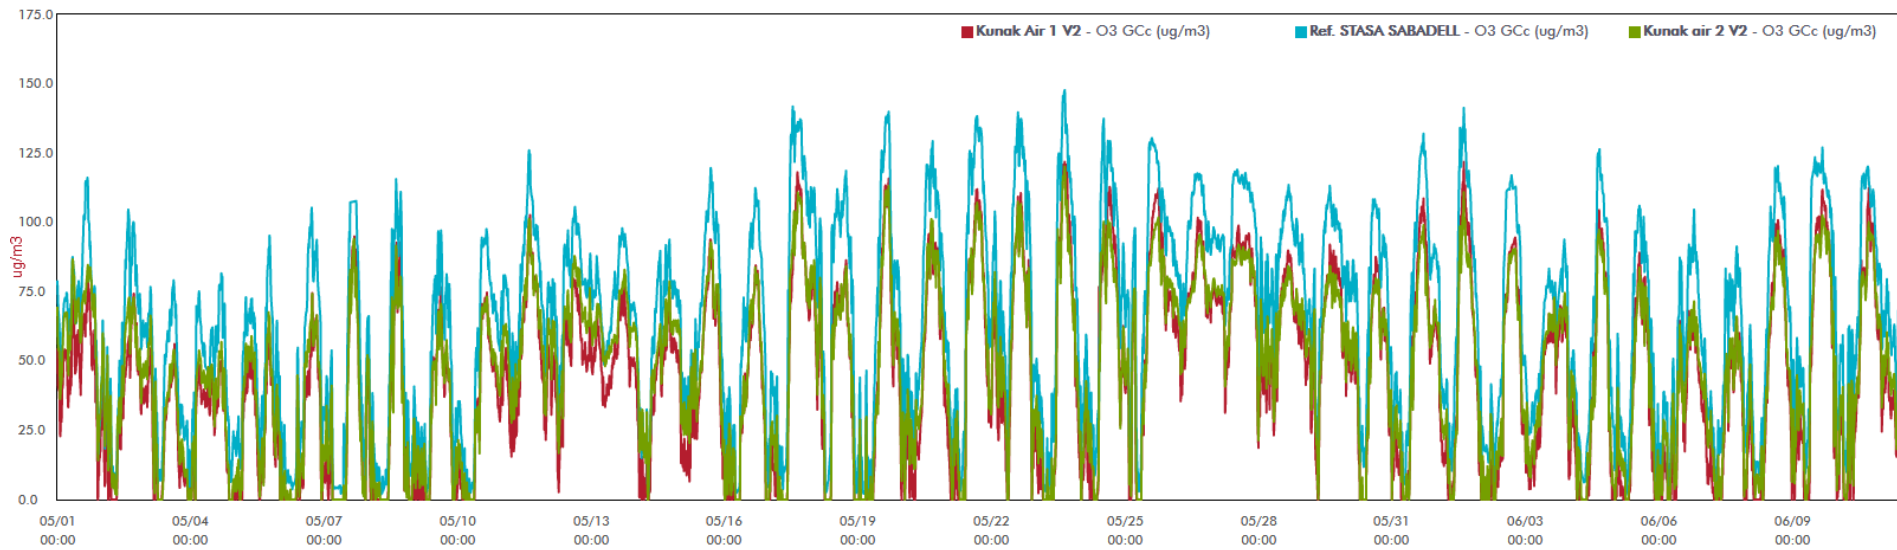


Comments: Excellent correlation between KUNAKAIR and reference instrument. Both devices perform very well, with similar trend variations. There is a small baseline offset producing lower average values that can be corrected to increase accuracy with a baseline calibration.

Version: KUNAKAIR V2.





Kunak Air 1 V2

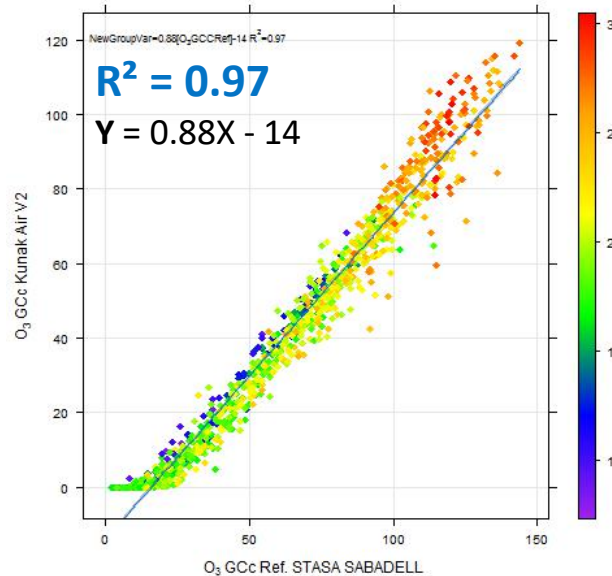

Kunak Air 2 V2

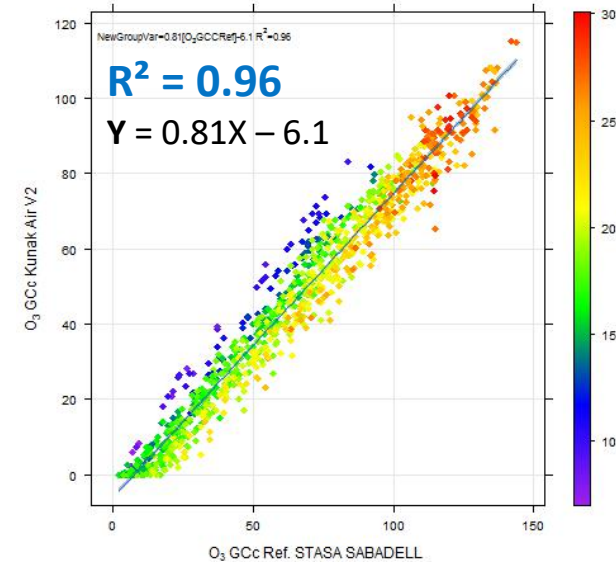

Time variation of two Kunak Air V2 and Ref. Torneo : O₃ GCc

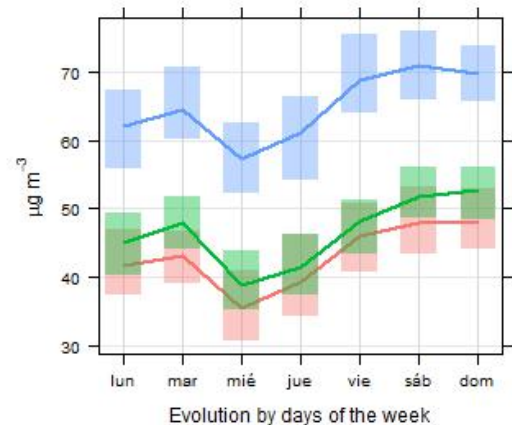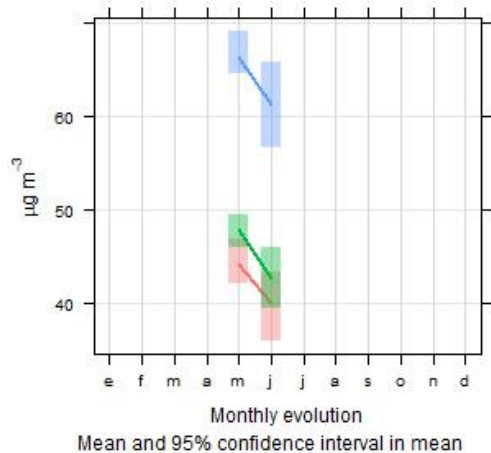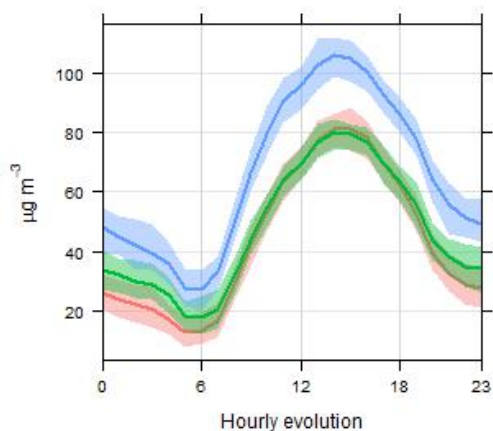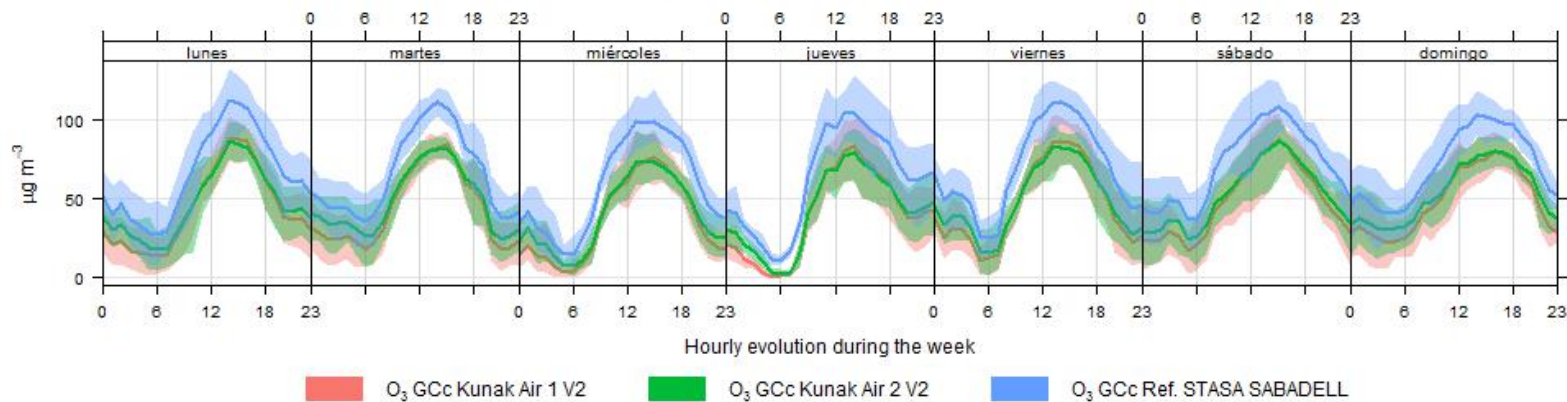

Device	R ²	ACCY (µg/m ³)	90% CONF. (µg/m ³)	AVG. GC. REF (µg/m ³)	AVG. GC. DUT (µg/m ³)	AV REF/DUT
KA 1	0.97	22.03	29.86	65	43.13	99.4 / 100
KA 2	0.96	18.58	30.01	65	46.57	99.4 / 100